


Interson USB Veterinary Endocavity VE 5.0 MHz B-Scan Ultrasound Probe System

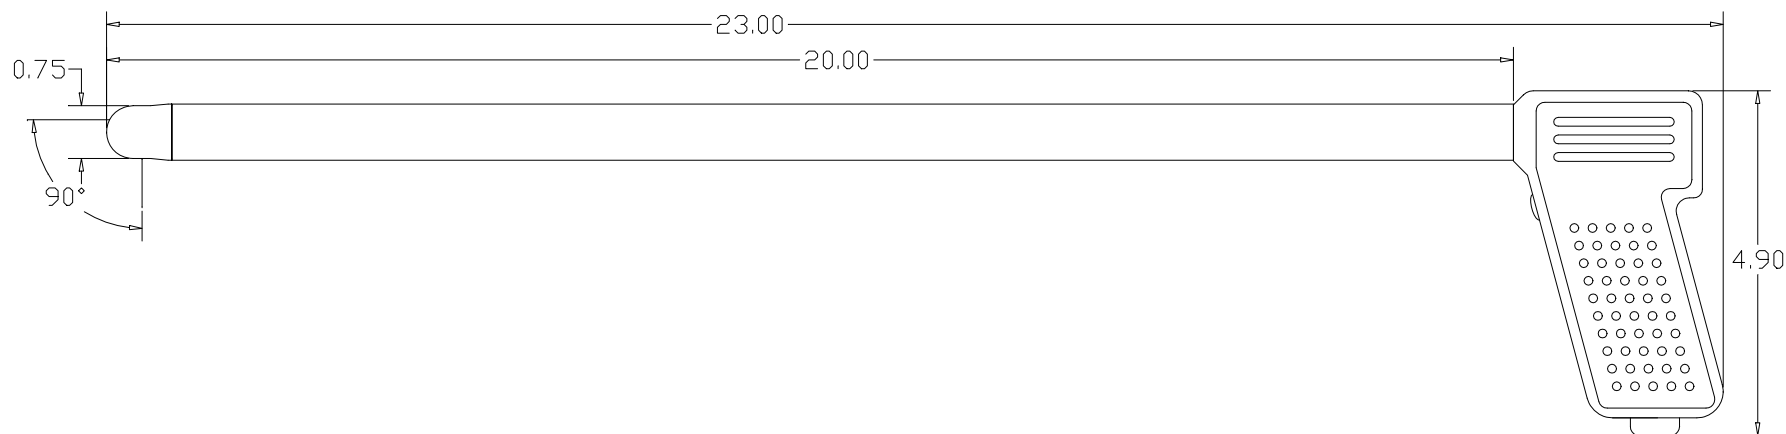

PROBE SPECIFICATION	SYSTEM REQUIREMENTS
3.5 - 5.0 MHz ($f_c = 5.0$ MHz) Real Time Images	Processor Speed ≥ 1 GHz
Scan Angle: 90° ,Semi-Side Fire	DDR SDRAM ≥ 512 MB
Focal Point: 6.0 cm	Windows XP
Scan Depth (max): 20 cm	USB 2.0
Patient contact sector length: 25 mm	
Freeze Button	
Cine Loop with Pre & Post Trigger Save Modes	

06/2007